

Product Datasheet

Laser Gas Detection OEM Module LGD F200P2-H Series

1 General description

Axetris is offering Laser Gas Detection (LGD) modules with exceptional advantages and value for the customer. Tunable Diode Laser Spectrometry (TDLS), enhanced by proprietary technology, is used for the measurement of CO₂, NH₃, CH₄, HCl, (H₂O). The modules are designed for integration by Original Equipment Manufacturers (OEMs), active in the field of gas detection and monitoring in diverse industries.

The **LGD F200** series is based on a contactless, near-infrared absorption measurement of the target gas. The systems are self-contained, ready-to-use OEM modules, using a flow-through cell set-up for extractive measurements. The slightly bigger LGD F200 (H) version features optional cell heating up to 220°C for hot gas measurements in process control and environmental compliance related applications.

The system has micro-processor-driven read-out electronics and digital and/or analog data outputs for industry-standard connectivity. Proprietary electronic lock-in technology allows separating gas absorption information from electro-optical system information, eliminating the need for a physical reference channel and providing continuous sensor status monitoring. Low maintenance operation and long life time provide customers with exceptionally low cost-of-ownership and make the LGD F200 the ideal instrument for your OEM applications.

Main applications

- Process control:
SCR, incineration & combustion processes, ...
- Emission monitoring:
Power generation, engine development, waste incineration furnaces, ...
- Environmental monitoring:
Landfill & green-house gases, livestock, ...
- Chemical engineering:
Production control & monitoring ...
- Safety:
Leak detection, refrigeration, toxic gases, ...
- Climate control & monitoring:
Livestock, climate chambers & rooms, ...



Key features

- Made for easy integration by OEMs
- Optical, contact-less measurement
- Accurate laser-diode electro-optics
- High selectivity
- Fast response
- Self-contained
- Continuous sensor status monitoring
- Low maintenance
- Low cost-of-ownership
- 10-30V power supply
- Digital and analog data interfaces
- Hot-gas measurement up to 170/190/220°C

2 Execution specifications

2.1 Gas detection specifications for LGD F200P2-H NH₃ SCR Industrial

Important:

Reference conditions: External: 20°C – 23°C, 920 -1020 hPa, 40 to 50% r.H.; Gas & cell: Incoming gas temperature at 190°C, measurement cell at 190°C/220°C, 10% absolute H₂O in the measurement gas.

Parameter	Unit	Value / Range
Gas	-	NH ₃
Maximum Range	ppm	0 – 100
Minimum Range	ppm	0 – 20
		calibration to full scale (FS) range, standard is 100 ppm, for safety reasons max. calibration to 100 ppm (linearity up to 500 ppm, no warranty of precision)
Accuracy ¹	-	± 2.0 % full scale reading depending on integration stability (temperature & pressure)
Precision ² 2σ	ppm	1.8 with 1 s averaging time ³ 0.8 with 10 s averaging time ³
Linearity & Repeatability	-	included in the accuracy
Gas cross talk/interference	-	to H ₂ O: < 0.05 ppm of reading NH ₃ per % H ₂ O
Displayed resolution	ppm	0.01 (negative values can also be displayed)
Refresh rate	s	1 (integration time can be selected, max. 600 s)
T ₉₀ time	s	2 (at gas flow rate of 3 L/min)
Recommended stabilized Integration Temperature	°C	20 ... 45 (as narrow as possible, application defined)
Cell temperature range	°C	190/220
Incoming gas temperature	°C	same as set cell temperature
Max. surface temp. housing	°C	65 (@190°C) / 75 (@220°C)
Meas. gas max. humidity	% abs. H ₂ O	30
Input for external parameter compensation	-	pressure, temperature or matrix gas concentration (optional)

¹ **Accuracy:** The accuracy is defined as the difference between the mean response during a 2 min time interval and the reference value at reference conditions. Variations of the operating temperature and pressure can affect the accuracy of the system.

² **Precision:** The precision is defined as 2 times the standard deviation σ of a 2 min measurement at stable reference conditions over the full measuring range. The precision of the system can be improved by mean of averaging.

³ **Averaging time:** An exponential moving average (EMA) is applied on measured concentration values. The averaging time expresses the period of time of past measurements considered to compute the next averaged value. The averaging time can be set up to 600 s.

2.2 Gas detection specifications for LGD F200P2-H NH3 QAL1 compliant

Important:

Reference conditions: External: 20°C – 23°C, 920 -1020 hPa, 40 to 50% r.H.; Gas & cell: Incoming gas temperature at 190°C, measurement cell at 190°C, 10% absolute H₂O in the measurement gas.

Parameter	Unit	Value / Range
Gas	-	NH ₃ / H ₂ O
NH ₃	ppm	
Minimum Range		0 – 15
Extended Range		0 – 50
H ₂ O	% vol.	
Minimum Range		0 – 30
Maximum Range		0 – 40
Accuracy ¹	-	± 2.0 % full scale reading depending on integration stability (temperature & pressure)
NH ₃ Precision ² 2σ	ppm	0.2 with 60 s averaging time ³
H ₂ O Precision ² 2σ	ppm	1000 with 60 s averaging time ³
Linearity & Repeatability	-	included in the accuracy
Cross-sensitivity NH ₃	-	< 4.0 % (15% vol. H ₂ O)
Cross-sensitivity H ₂ O		< 4.0 % (15% vol. CO ₂ , 21% vol.O ₂)
Displayed resolution	ppm	0.01 (negative values can also be displayed)
Refresh rate	s	2 (integration time can be selected, max. 600 s)
T ₉₀ time	s	10 (at gas flow rate of 3 L/min)
Recommended stabilized Integration Temperature	°C	20 ... 45 (as narrow as possible, application defined)
Cell temperature range	°C	190
Incoming gas temperature	°C	same as set cell temperature, max. 190
Max. surface temp. housing	°C	65
Input for external parameter compensation	-	pressure, temperature or matrix gas concentration (optional)

¹ **Accuracy:** The accuracy is defined as the difference between the mean response during a 2 min time interval and the reference value at reference conditions. Variations of the operating temperature and pressure can affect the accuracy of the system.

² **Precision:** The precision is defined as 2 times the standard deviation σ of a 2 min measurement at stable reference conditions over the full measuring range. The precision of the system can be improved by mean of averaging.

³ **Averaging time:** An exponential moving average (EMA) is applied on measured concentration values. The averaging time expresses the period of time of past measurements considered to compute the next averaged value. The averaging time can be set up to 600 s.

2.3 Gas detection specifications for LGD F200P2-H NH3 SCR Vehicle

Important:

Reference conditions: External: 50°C, 920 -1020 hPa, 40 to 50% r.H.; Gas & cell: Incoming gas temperature at 170°C, measurement cell at 170°C, 10% absolute H₂O in the measurement gas.

Parameter	Unit	Value / Range
Gas	-	NH ₃
Principle of detection	-	Tunable Diode Laser Spectrometry (TDLS)
Range	ppm	0 – 1500 Standard calibration is 100 ppm, for safety reasons
Accuracy ¹	-	± 1 ppm (0-99ppm) +/-1% of Reading (100 – 999ppm) +/- 3% of Reading (1000 – 1500ppm)
Lower Detection Limit ²	ppm	1 with 1 s averaging time ³
Precision ⁴ 2σ	ppm	1.8 or 1% of Reading, whichever is larger with 1 s averaging time ³
Linearity & Repeatability	-	included in the accuracy
Gas cross talk/interference	-	to H ₂ O: < 0.05 ppm NH ₃ per % H ₂ O
Displayed resolution	ppm	0.01 (negative values can also be displayed)
Refresh rate	s	1 (integration time can be selected, max. 600 s)
T ₉₀ time	s	2 (at gas flow rate of 3 L/min)
Recommended stabilized Integration Temperature	°C	25 ... 50 (as narrow as possible, application defined)
Cell temperature range	°C	170
Incoming gas temperature	°C	same as set cell temperature
Max. surface temp. housing	°C	60
Meas. gas max. humidity	% abs. H ₂ O	40
Input for external parameter compensation	-	pressure, temperature or matrix gas concentration (optional)

¹ **Accuracy:** The accuracy is defined as the difference between the mean response during a 2 min time interval and the reference value in dry conditions. Variations of the operating temperature and pressure can affect the accuracy of the system.

² **Lower Detection Limit:** The LDL is defined as 2 times the standard deviation σ of a 2 min measurement at stable reference conditions 0ppm setpoint. It can be improved by mean of averaging.

³ **Averaging time:** An exponential moving average (EMA) is applied on measured concentration values. The averaging time expresses the period of time of past measurements considered to compute the next averaged value. The averaging time can be set up to 600 s.

⁴ **Precision:** The precision is defined as 2 times the standard deviation σ of a 2 min measurement at stable reference conditions at full scale. The precision of the system can be improved by mean of averaging.

2.4 Gas detection specifications for LGD F200P2-H H2O

Important:

Reference conditions: External: 20°C – 23°C, 920 -1020 hPa, 40 to 50% r.H.; Gas & cell: Incoming gas temperature at 190°C, measurement cell at 190°C, 10% absolute H₂O in the measurement gas.

Parameter	Unit	Value / Range
Gas	-	H ₂ O
Principle of detection	-	Tunable Diode Laser Spectrometry (TDLS)
Range	% vol.	0 – 30 calibration to full scale (FS) range
Accuracy ¹	% vol.	± 0.5 absolute, depending on integration stability (temperature & pressure)
Precision ² 2σ	% vol.	0.2 with 1 s averaging time ³ 0.1 with 10 s averaging time ³
Linearity & Repeatability	-	included in the accuracy
Displayed resolution	ppm	0.01 (negative values can also be displayed)
Refresh rate	s	1 (integration time can be selected, max. 600 s)
T ₉₀ time	s	2 (at gas flow rate of 3 L/min)
Recommended stabilized Integration Temperature	°C	20 ... 45 (as narrow as possible, application defined)
Cell temperature range	°C	190
Incoming gas temperature	°C	same as set cell temperature, max. 190
Max. surface temp. housing	°C	65
Meas. gas max. humidity	% abs. H ₂ O	30
Input for external parameter compensation	-	pressure, temperature or matrix gas concentration (optional)

¹ **Accuracy:** The accuracy is defined as the difference between the mean response during a 2 min time interval and the reference value at reference conditions. Variations of the operating temperature and pressure can affect the accuracy of the system.

² **Precision:** The precision is defined as 2 times the standard deviation σ of a 2 min measurement at stable reference conditions over the full measuring range. The precision of the system can be improved by mean of averaging.

³ **Averaging time:** An exponential moving average (EMA) is applied on measured concentration values. The averaging time expresses the period of time of past measurements considered to compute the next averaged value. The averaging time can be set up to 600 s.

2.5 Gas detection specifications for LGD F200P2-H HCl

Important:

Reference conditions: External: 20°C – 23°C
920 -1020 hPa
40 to 50% r.H.;

Gas & cell: Incoming gas temperature at 190°C
measurement cell at 190°C
10% absolute H₂O in the measurement gas.

Parameter	Unit	Value / Range
Target Gas	-	HCl
Principle of detection	-	Tunable Diode Laser Spectrometry (TDLS)
Measuring Range	ppm	0 – 50 (linearity up to 500 ppm, no warranty of precision)
Lowest Detection Limit ¹ 2σ	ppm	< 0.4 with 10s averaging time
Precision ² 2σ	ppm	< 0.6 with 10 s averaging time ³
Accuracy ⁴	ppm	± 2
Sampling rate	Hz	0.5
T ₉₀ time	s	20 (at gas flow rate of 3 L/min)
Resolution	ppm	0.01
Linearity & Repeatability	-	included in the accuracy
Cross interference	-	to H ₂ O: < 0.05 ppm of reading HCl per % H ₂ O
Cell temperature range	°C	190
Meas. gas max. humidity	% abs. H ₂ O	30

¹ **Lowest Detection Limit (LDL):** The LDL is defined as 2 times the standard deviation σ evaluated over a time period of a 2 min measurement at stable reference conditions with set point 0 ppm. The LDL of the system can be improved by mean of averaging.

² **Precision:** The precision is defined as 2 times the standard deviation σ of a 2 min measurement at stable reference conditions over the full measuring range. The precision of the system can be improved by mean of averaging.

³ **Averaging time:** An exponential moving average (EMA) is applied on measured concentration values. The averaging time expresses the period of time of past measurements considered to compute the next averaged value. The averaging time can be set up to 600 s.

⁴ **Accuracy:** The accuracy is defined as the difference between the mean response during a 2 min time interval and the reference value at reference conditions. Variations of the operating temperature and pressure can affect the accuracy of the system.

2.6 Environmental conditions

Parameter	Unit	Value / Range
Usage	-	Interior use
Maximum operating temperature range	°C	15 ... 50
Operating humidity	% r.H.	0 ... 99, non-condensing
Operating pressure	mbar	800 ... 1100
Storage temperature	°C	-40 ... 80
Storage humidity	% r.H.	0 ... 99, non-condensing
Emission level L _{pa} *	dB	<70

*specification for CE conformity

2.7 Mechanical characteristics

Parameter	Unit	Value / Range
Measurement cell	-	Flow-through set-up
Standard cell length	mm	200
Standard cell volume	mL	15
Maximum measurement gas flow rate (Minimum)	mL / min	5'000 (1'500)
Dimensions housing, heated (H) version:	mm ³	380 x 122 x 78
Approx. weight, heated (H) version	kg	3.3
Inlet / outlet connectors, measurement gas	mm	6 O.D., Swagelok
Inlet / outlet connectors, purge gas (optional)	mm	6 O.D., push-in fitting

2.8 Electrical characteristics

Parameter	Unit	Value / Range
Voltage supply DC Min. / Max. rating	V	10 ... 30 (max. ripple \pm 100mV, max. current 0.5A, DC inrush current limitation 1A, reverse battery protection)
System power consumpt.	W	< 2
Max. cell heating power consumption, (H) version	W	100
Start-up time	s	30
Warm-up time		
Cell heating to 190°C	min.	30 (starting at 25°C)
Cell heating to 220°C	min.	40 (starting at 25°C)
Stable operation after	min	60 (at 190°C cell temperature)


2.9 Communication interface

Parameter	Unit	Value / Range
Digital interface RS232	-	Protocol available; standard.
Analog interface Current output	mA	4...20, 12-bit resolution (on 0 ... 25 mA); standard
Voltage output	V	0...5, 12-bit resolution; on request
Alarm	-	Customer configurable and definable

3 Connector assignments

3.1 System Power / User interface connector assignments

Figure 1: Head view electronics housing.
System Power / User interface terminal connector assignment.

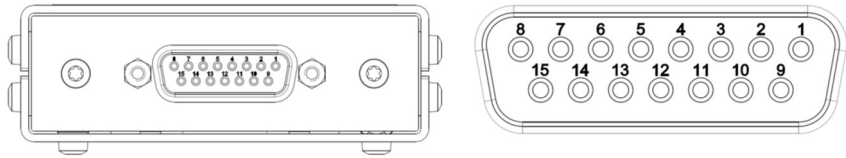


Connector assignment:

	Pin	Name	Description
Power Supply	1	POWER IN	Power supply 10 ... 30V
	2	GND IN*	Power supply ground
	3	SHIELD	DB 15 Connector - Housing
Digital Interfaces	6	GND*	Ground serial communication
	7	RS232 TX	UART serial communication
	8	RS232 RX	UART serial communication
	14	N/A	Not used
Relay Alarms	15	N/A	Not used
	4	ALARM 1	On/Off signal at defined conditions for relay control, hardware watchdog, etc
	5	ALARM 2	On/Off signal at defined conditions for relay control, hardware watchdog, etc
	11	ALARM 3	HW watchdog, firmware error and warnings
	12	VCC RELAY	Relay power supply: 10 V < Vcc Relay < 30 V; max. 0.75 A
Analog Interface	13	GND*	Ground, relay alarms
	9	ANALOG GND*	Analog ground
	10	ANALOG OUT	Analog output Factory setting: output current (4-20mA); output voltage (0-5V) on request only

* same potential

3.2 Measurement cell heater connector assignment

Figure 2: Cell heater screw terminal connector assignment.
Head view electronics housing.

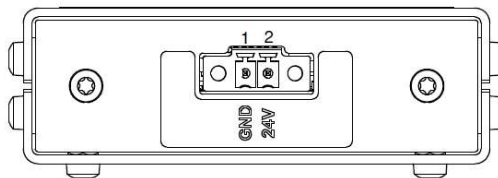

Connector assignment:

Pin	Name	Description
1	GND	Power ground
2	24V	Power supply 24V, Consumption: < 96W

4 Mechanical dimensions

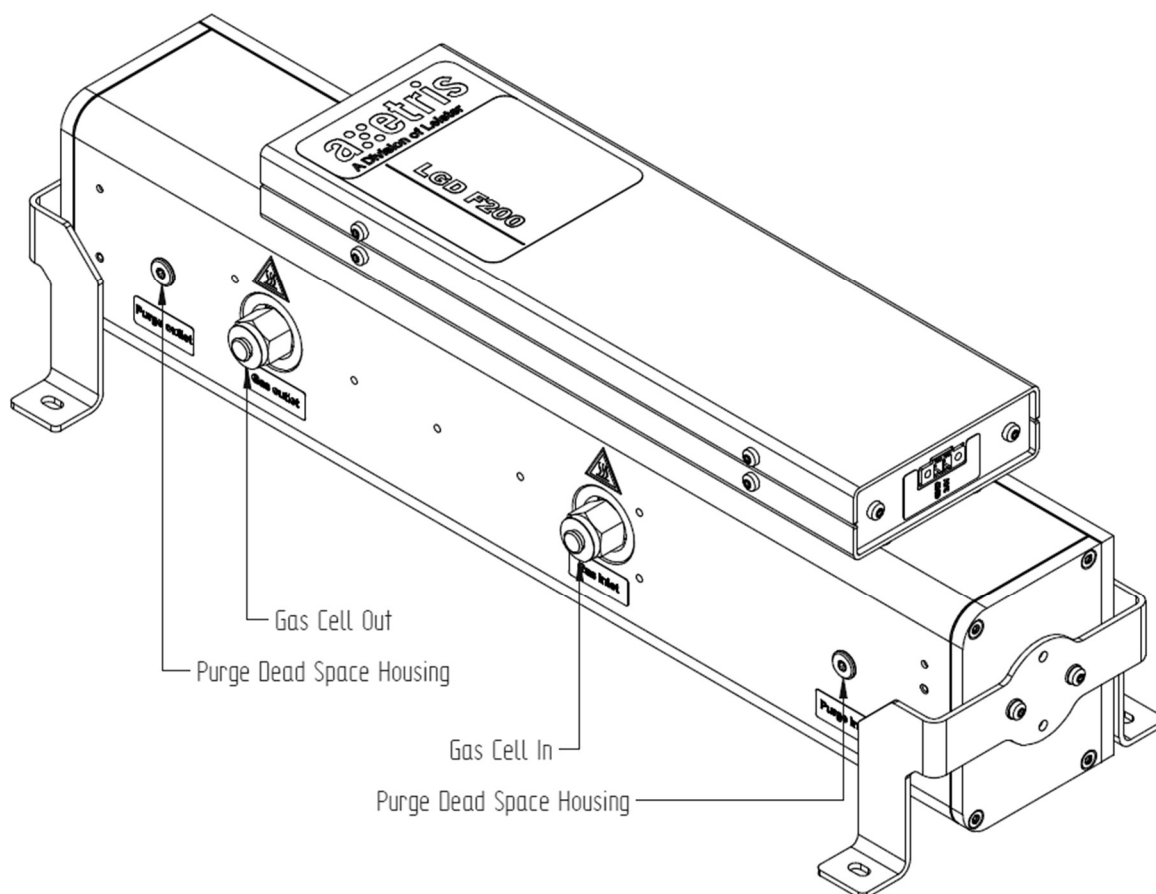


Figure 3: General view of the LGD F200P2 H sensor

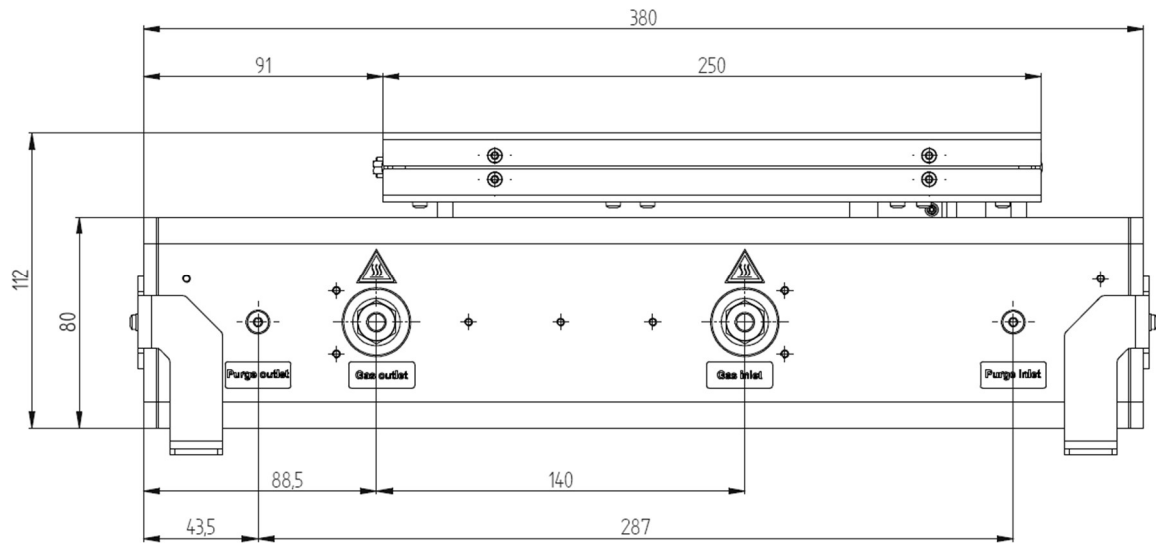


Figure 4: Side view, with gas connectors. Dimensions in mm

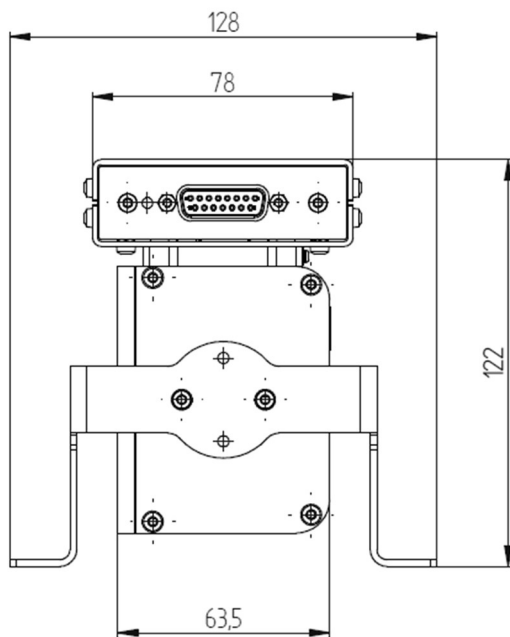


Figure 5: Front view. Dimensions in mm

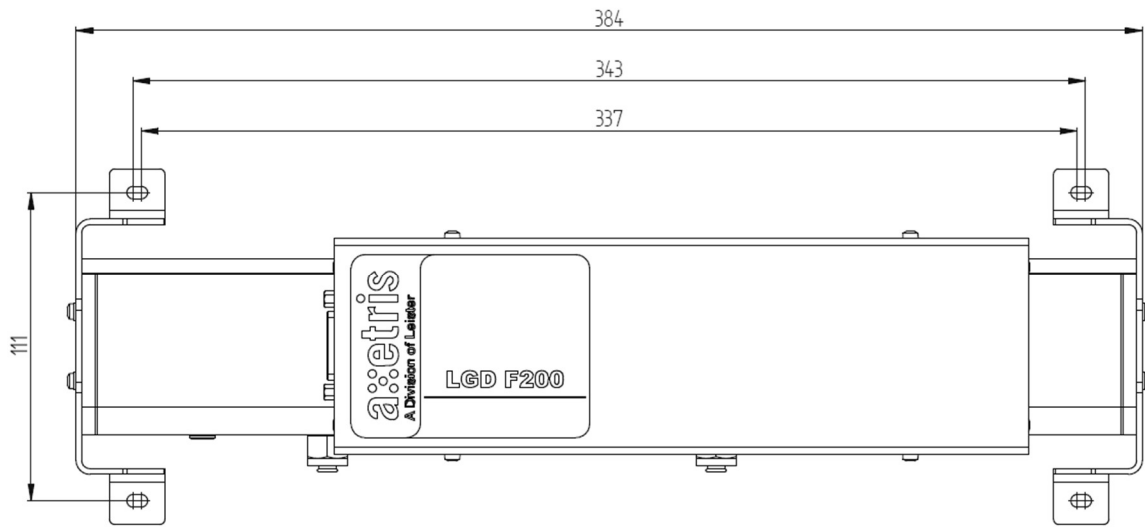


Figure 6: Top view. Dimensions in mm

5 Certifications

Type	Standard / Regulation	Limits
LGD F200P2 Platform conformity	REACH, CE	
Safety of laboratory products	EN/IEC 61010	
Safety of laser products	EN/IEC 60825-1	
EMC	EN/IEC 61326-1	Immunity test requirements for equipment intended for use in industrial locations
Shock	EN60068-2-27	150m/s ² , half sinus, 11ms, max acceleration 15g, 18 cycles
Vibration	EN60068-2-6	5 ... 50Hz, amplitude 0.35mm, 1 octave /min, 2h per orientation (total 18 Frequency cycle)
Electronics conformity	RoHS / WEEE	

6 Caution

6.1 Product damage

- Read all instructions carefully before using the device.
- The LGD F200P2 H laser gas detection modules are calibrated for a particular gas and concentration range. Do not use the sensor outside of its specifications.
- The sensor is not suited for measuring gases with a dust load. The incoming measurement gas must be conditioned in order to avoid dust and condensation of liquid in the sensor. Gas loaded with particles or other substances can eventually contaminate the cell and make it necessary to service the instrument.
- The appliance must not be used in damp or wet surroundings.
- Use only accessories that are indicated in the instructions for use or are recommended by the manufacturer.
- Failure to comply with these instructions could result in product damage.

6.2 Danger of life

- The sensor must not be used with flammable or explosive gases or mixtures.
- Unprofessional gas handling can cause injury or death. The use of gas detection modules should only be performed by qualified personnel
- Do not use this product as safety or emergency stop device or in any other application where failure of the product could result in personal injury or death.

© 2019 AXETRIS AG – Company of the Leister Group

Contact

Headquarters:
Axetris AG, Switzerland
Schwarzenbergstrasse 10
CH-6056 Kaegiswil
Switzerland
phone: +41 41 662 76 76
fax: +41 41 662 75 25
axetris@axetris.com
www.axetris.com

USA:
Leister Technologies LLC
1275 Hamilton Parkway
Itasca, IL 60143
United States
phone: +1 630 760 1000
fax: +1 630 760 1001
axetris.usa@axetris.com
www.axetris.com

China:
Leister Technologies Ltd.
Building 11, 155 Yuanke
Road
Xinzhuang Industry Park
Shanghai 201109 PR China
phone: +86 21 6442 2398
fax: +86 21 6442 2338
axetris@axetris.cn
www.axetris.cn

Japan:
Leister Technologies KK
Shinyokohama Bousei Bldg
1F
3-20-12, Shinyokohama,
Kohoku-ku
Yokohama 222-0033 /
Japan
phone: +81 45 477 36 37
fax: +81 45 477 36 38
axetris@axetris.jp
www.axetris.jp

7 Important Notice / Disclaimer

The information furnished by Axetris is believed to be correct and accurate. However, Axetris shall not be held liable to recipient or any third party of any damages, including but not limited to personal injury, property damage, loss of profits, loss of use, interrupt of business or indirect, special incidental or consequential damages, of any kind, in connection with or arising out of the furnishing, performance or use of technical data herein. No obligation or liability to recipient or any third party shall arise or flow out of Axetris rendering of technical or other services. While due caution has been exercised in the production of this document, possible errors and omissions are unintentional.

8 Axetris Certifications

Axetris is an ISO 9001 certified company. The LGD F200P2 H module is CE and RoHS 2 compliant.



CLASS 1 LASER PRODUCT
(classified according to SN EN 60825:1:2014)

Swiss Made Quality. Axetris is an **ISO 9001** certified enterprise. Specifications are subject to change without prior notice